


External Standard Report

Data File: D:\Enterprise\RDGroup3\Result\032511.seq.rslt\001.dat
 Method: D:\Enterprise\RDGroup3\Method\RLM-Calibration.met
 Acquired: 3/25/2011 3:00:15 PM (GMT -04:00)
 Printed: 3/28/2011 1:37:22 PM (GMT -04:00)

Sample Amt: 1
 Multiplier: 1

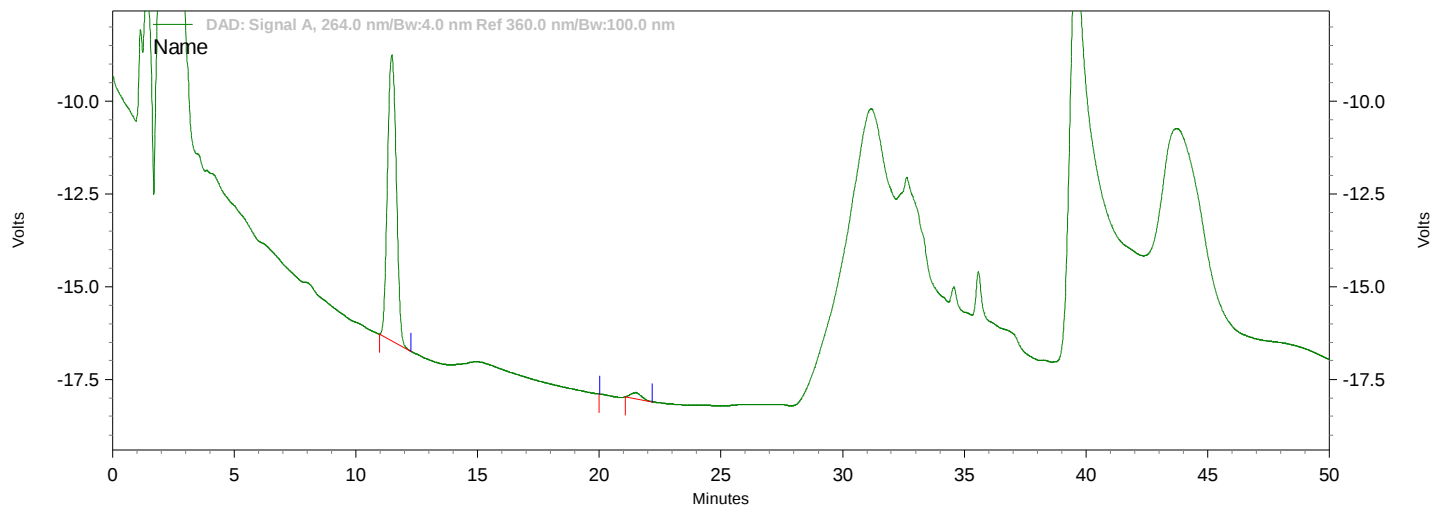

Channel A

DAD: Signal A, 264.0
 nm/Bw:4.0 nm Ref 360.0
 nm/Bw:100.0 nm Results

Name	Time	Area	Amount
Pre-cacitriol			0.000 BDL
	11.467	26051744	0.000
Unknown-1			0.000 BDL
Calcitriol			0.000 BDL
	20.000	0	0.000
Unknown-2			0.000 BDL
	21.487	669227	0.000

Totals		26720971.000000	0.000000
--------	--	-----------------	----------