


External Standard Report

Data File: D:\Enterprise\RDGroup3\Result\032511.seq.rslt\002.dat
Method: D:\Enterprise\RDGroup3\Method\RLM-Calibration.met
Acquired: 3/25/2011 3:54:13 PM (GMT -04:00)
Printed: 3/28/2011 1:37:28 PM (GMT -04:00)

Sample Amt: 1

Multiplier: 1

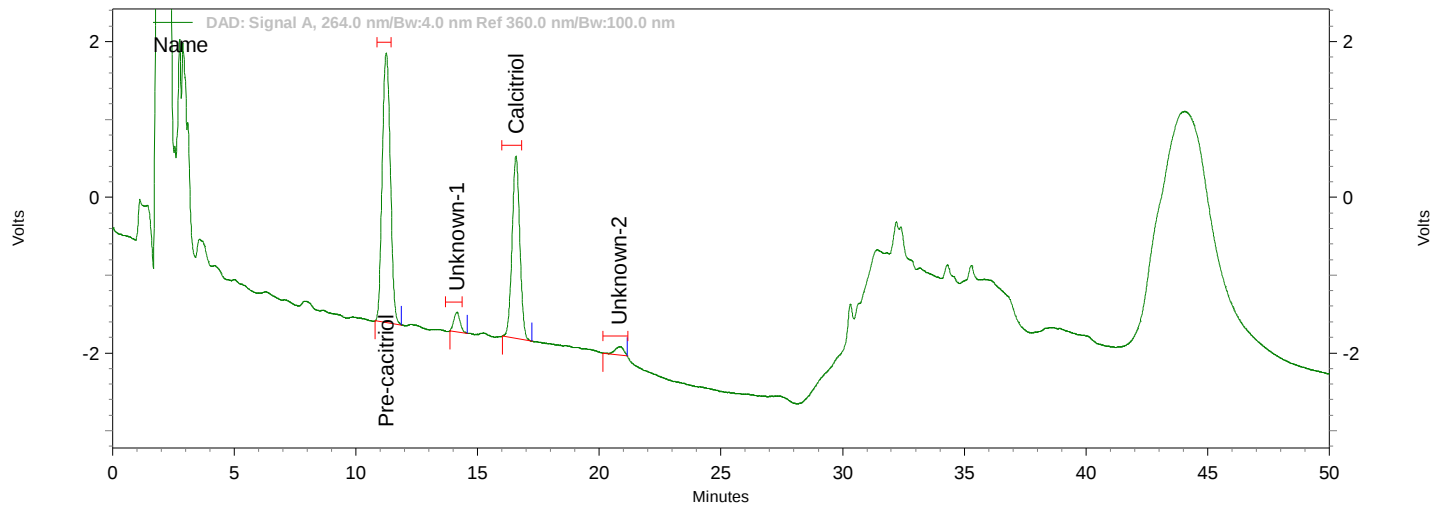

Channel A

DAD: Signal A, 264.0
nm/Bw:4.0 nm Ref 360.0
nm/Bw:100.0 nm Results

Name	Time	Area	Amount
Pre-cacitriol	11.240	10788724	0.144
Unknown-1	14.147	608738	0.008
Calcitriol	16.573	6963560	0.093
Unknown-2	20.813	365560	0.005

Totals		18726582.000000	0.249640
--------	--	-----------------	----------