


External Standard Report

Data File: D:\Enterprise\RDGroup3\Result\032511.seq.rslt\003-Rep2.dat
 Method: D:\Enterprise\RDGroup3\Method\RLM-Calibration.met
 Acquired: 3/25/2011 5:42:12 PM (GMT -04:00)
 Printed: 3/28/2011 1:37:44 PM (GMT -04:00)

Sample Amt: 1
 Multiplier: 1

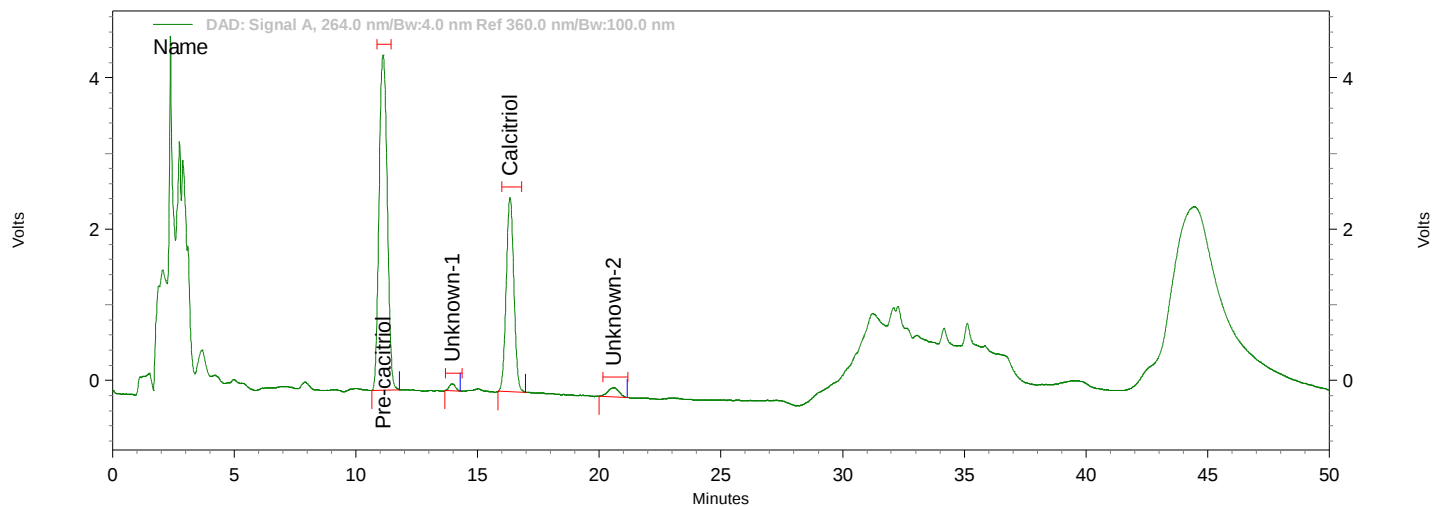

Channel A

DAD: Signal A, 264.0
 nm/Bw:4.0 nm Ref 360.0
 nm/Bw:100.0 nm Results

Name	Time	Area	Amount
Pre-cacitriol	11.113	13978572	0.000 CAL
Unknown-1	13.953	230114	0.000 CAL
Calcitriol	16.327	7504330	0.100 CAL
Unknown-2	20.573	522476	0.000 CAL

Totals		22235492.000000	0.100000 CAL
--------	--	-----------------	-----------------