


External Standard Report

Data File: D:\Enterprise\RDGroup3\Result\032511.seq.rslt\003-Rep3.dat
Method: D:\Enterprise\RDGroup3\Method\RLM-Calibration.met
Acquired: 3/25/2011 6:36:09 PM (GMT -04:00)
Printed: 3/28/2011 1:37:52 PM (GMT -04:00)

Sample Amt: 1
Multiplier: 1

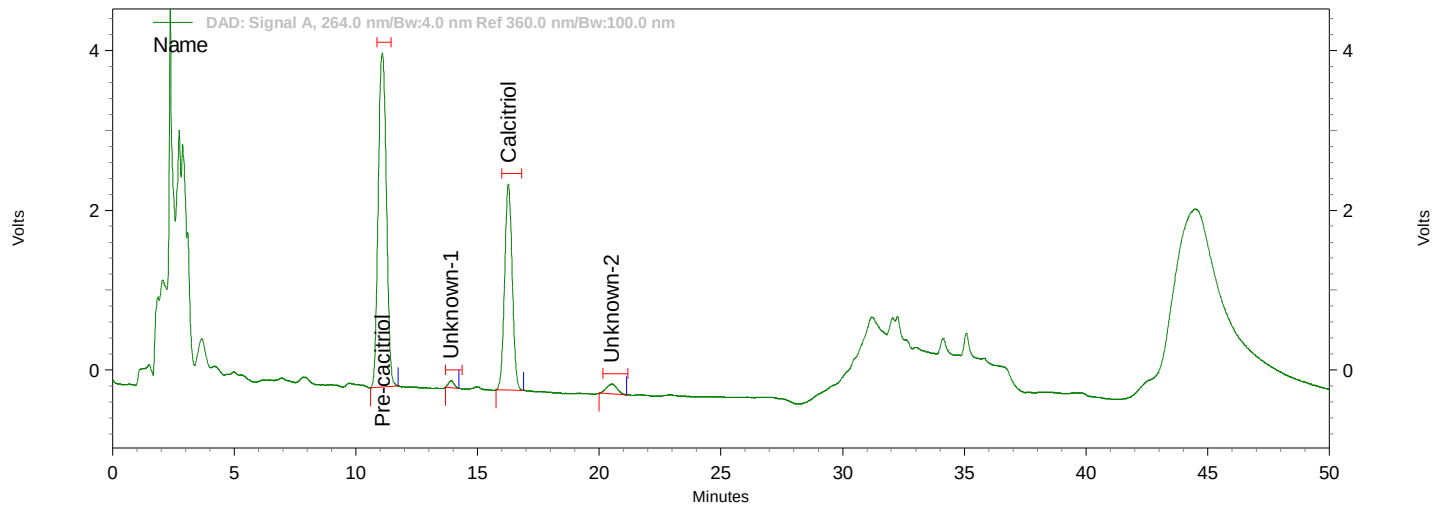

Channel A

DAD: Signal A, 264.0
nm/Bw:4.0 nm Ref 360.0
nm/Bw:100.0 nm Results

Name	Time	Area	Amount
Pre-cacitriol	11.080	13121544	0.000 CAL
Unknown-1	13.913	193219	0.000 CAL
Calcitriol	16.267	7494630	0.100 CAL
Unknown-2	20.493	505640	0.000 CAL

Totals		21315033.000000	0.100000 CAL
--------	--	-----------------	-----------------