


External Standard Report

Data File: D:\Enterprise\RDGroup3\Result\032511.seq.rslt\006.dat
 Method: D:\Enterprise\RDGroup3\Method\RLM-Calibration.met
 Acquired: 3/25/2011 10:11:49 PM (GMT -04:00)
 Printed: 3/28/2011 1:38:36 PM (GMT -04:00)

Sample Amt: 1
 Multiplier: 1

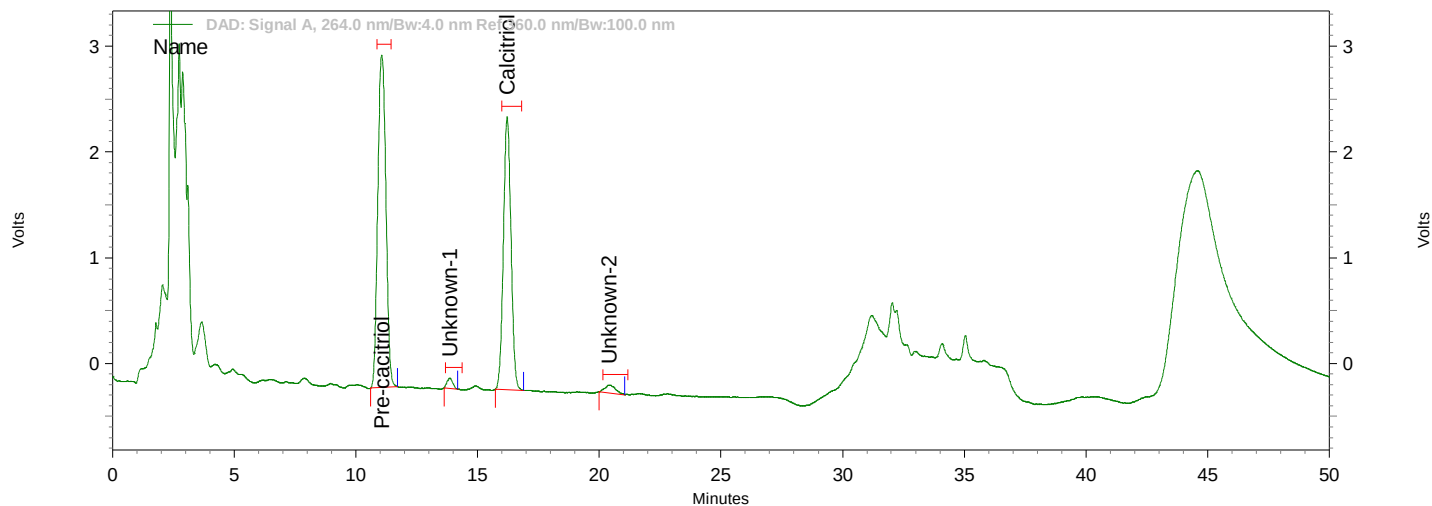

Channel A

DAD: Signal A, 264.0
 nm/Bw:4.0 nm Ref 360.0
 nm/Bw:100.0 nm Results

Name	Time	Area	Amount
Pre-cacitriol	11.060	9801950	0.131
Unknown-1	13.847	211737	0.003
Calcitriol	16.213	7517218	0.100
Unknown-2	20.400	293794	0.004

Totals		17824699.000000	0.237617
--------	--	-----------------	----------