


External Standard Report

Data File: D:\Enterprise\RDGroup3\Result\032511.seq.rslt\007.dat
 Method: D:\Enterprise\RDGroup3\Method\RLM-Calibration.met
 Acquired: 3/25/2011 11:05:45 PM (GMT -04:00)
 Printed: 3/28/2011 1:38:42 PM (GMT -04:00)

Sample Amt: 1
 Multiplier: 1

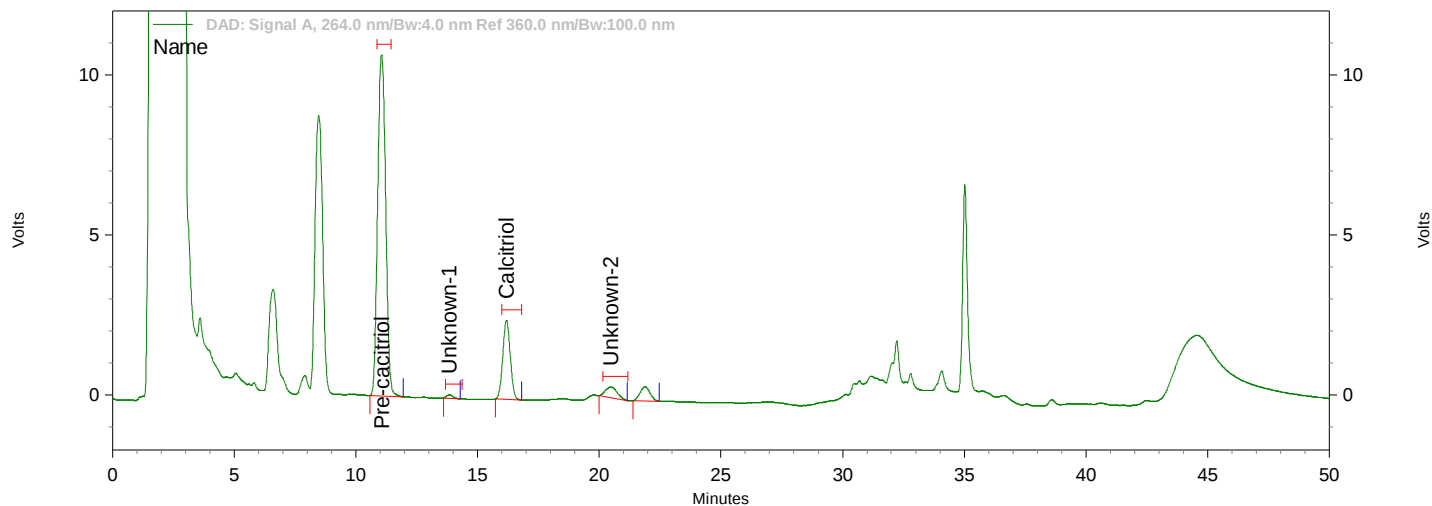

Channel A

**DAD: Signal A, 264.0
 nm/Bw:4.0 nm Ref 360.0
 nm/Bw:100.0 nm Results**

Name	Time	Area	Amount
Pre-cacitriol	11.047	32848122	0.438
Unknown-1	13.820	253496	0.003
Calcitriol	16.187	7120543	0.095
Unknown-2	20.473	1529520	0.020
	21.867	1672974	0.000

Totals		43424655.000000	0.556583
--------	--	-----------------	----------