


External Standard Report

Data File: D:\Enterprise\RDGroup3\Result\032511.seq.rslt\010.dat
Method: D:\Enterprise\RDGroup3\Method\RLM-Calibration.met
Acquired: 3/26/2011 1:47:35 AM (GMT -04:00)
Printed: 3/28/2011 1:39:00 PM (GMT -04:00)

Sample Amt: 1

Multiplier: 1

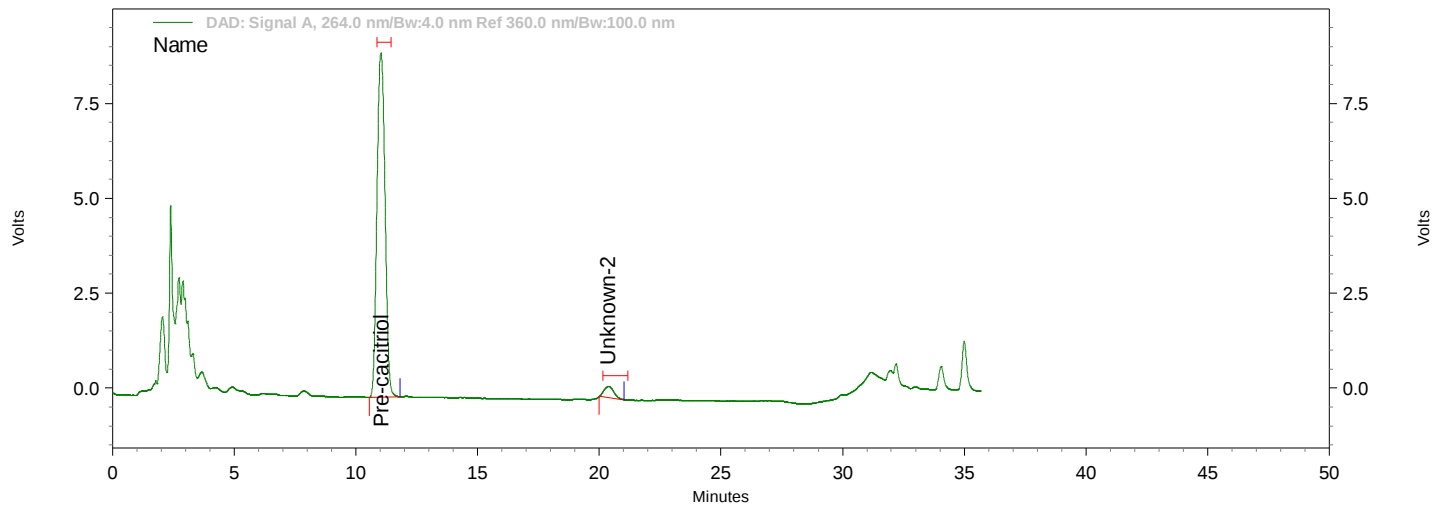

Channel A

DAD: Signal A, 264.0
nm/Bw:4.0 nm Ref 360.0
nm/Bw:100.0 nm Results

Name	Time	Area	Amount
Pre-cacitriol	11.020	28045961	0.374
Unknown-1			0.000 BDL
Calcitriol			0.000 BDL
Unknown-2	20.353	1089601	0.015

Totals		29135562.000000	0.388400
--------	--	-----------------	----------